1977 Author Index

(Asterisk indicates abstract)

Adabi, A. see Hambright, P.
Appledorn, C.R., Hallberg, J.R., and Knight, R.L. Unusual flood field image, 213
Armstrong, C. see Brown, T.

Bacharach, S.L. see Mack, B.A.
Barat, K., and Schwab, C. Deep and superficial venous thrombosis detection, 114*
Baron, K., Clay, B., Zimmer, A.M., and Pavel, D.G. Evaluation of commercial ^{99m}Tc-MAA, 111*
Bates, B.B., Rerych, S.K., and Jones, R.H. Exercise techniques for radionuclide angiocardiography, 112*
Battaglia, D.J., Burkhead, C., and Cianci, M. Statistical evaluation of radioimmunoassay normal range data, 101
Baumgartner, J. Improvement in the precision and accuracy of a commercially available insulin radioimmunoassay kit, 205
Becker, G.P. see Thorson, L.M.
Berg, R. see Burr, J.E.
Berger, H.J. see Pytlik, L.M.
Blonde, L. see Witherspoon, L.R.
Borer, J.S. see Mack, B.A.
Brahmaver, S.M.
see Lis, G.
see Washburn, R.
Brown, T., Armstrong, C., Brunsden, B.S., and Lands, E.L. Longitudinal multiplane emission tomography, 109*
Brunsden, B.S. see Brown, T.
Burkhead, C. see Battaglia, D.J.
Burr, J.E., and Berg, R. Radiation dose to hands from radiopharmaceutical—preparation vs injections, 158

Callahan, L. see Spicer, J.A.
Capuzzi, J.P. see Malmud, L.S.
Carretta, R.F. see Stankiewicz, C.J.
Chan, F.H. see Kowalsky, R.J.
Charkes, N.D. See Malmud, L.S.
Cherry, M. see Hambright, P.
Chilton, H.M. see Williams, R.C.
Christian, P.E. see Volz, E.M.
Cianci, M. see Battaglia, D.J.
Ciez, T. Diagnosis of cold thyroid nodules, 113*
Clark, N. see Tripses, K.
Clay, B. see Baron, K.
Conway, J.J. see Weiss, S.
Cradduck, T.D. Book review: *ICRU Report 25, Conceptual Basis for the Determination of Dose Equivalent,* 106
Cudworth, J.W. In-service education, 169
Czerwinski, B., and Ochart, M. Rectilinear tomographic scanner, 146

Dalton, J. see Washburn, R.
Dean, R.D. Book review: *The Basic Physics of Radiation Therapy,* 106
Dellwo, P.M. Cranial hyperotosis, 161
Deville, T. see Timpe, G.M.
Dhawan, V.M. see Rich, D.A.
Dubovsky, E.V. see Kontzen, F.N.
Dworkin, H.J. see Hill, J.C.

Fisher, R.S. see Malmud, L.S.
Floriddia, D.G. see Gunther, C.W.
Frank, P. see Koester, L.M.

Gallagher, J.H. see Hladik, W.B.
Garcia, E.V. see Koorji, A.H.
Gerson, M. Choosing a goodness-of-fit test, 217
Gibbs, W.D. see Hodges H.D.
Giga, J.L. see Stankiewicz, C.J.
Gors, R.F. Method for determining tomographic plane separation and detector distances for use with the Searle Pho/Con tomographic multiplane scanner, 152
Gottschalk, A. see Pytlik, L.M.
Grabowski, C. see Malmud, L.S.
Green, M.V. see Mack, B.A.
Green, W.R. ^{99m}Tc-GHT demonstration of a Dandy-Walker cyst, 85
Gunther, C.W., Wilkerson, S.V., and Floriddia, D.G. Dose calibrator performance and quality control, 168

Hallberg, J.R. see Appledorn, C.R.
Hambright, P., Adabi, A., Reid, J., Maitland, D., Press, H.C., and Cherry, M. Rapid spot test for stannous tin levels in ^{99m}Tc kits, 88
Hill, J.C., and Dworkin, H.J. Syringe apparatus for radiolabeling cells, 32
Hladik, W.B., Study, K.T., Gallagher, J.H., and Rhodes, B.A. QC of radiochemical purity by a rapid feedback system, 94
Hodges, H.D., and Gibbs, W.D. Radiation accident management, 46
Hodges, H.D., Holloway, S., and Gibbs, W.D. Reducing CO_2 inhalation in clinical pulmonary investigations, 211
Holloway, S. see Hodges, H.D.
Honeyman, J.C. Design criteria for a nuclear medicine department, 112*
Hopkins, G.B. see Kan, M.K.

Johnston, G.S. see Mack, B.A.
Johnston, R.E. see Kowalsky, R.J.
Jones, R.H. see Bates, B.B.
Jones, S.A. Nuclear medicine computer systems: a buyer's guide to current performance and future promise, 199

Kan, M.K., and Hopkins, G.B. Rib phantom for myocardial infarct scintigraphy, 50
Kan, M.K., and O'Sargent, D. Image quality in ^{99m}Tc-HSA cardiovascular imaging, 52
Kasecamp, W. see Mikesell, H.H.
Kirchhoff, K. see Tripses, K.
Knight, R.L. see Appledorn, C.R.
Koester, L.M., Frank, P., and Leeper, M.A. Effect of reduced Tc on scintillation camera imaging, 110*
Kontzen, F.N., Tobin, M., Dubovsky, E.V., and Tauxe, W.N. Comprehensive renal function studies, 81
Koorji, A.H., Garcia, E.V., and Maile, A. Photopeak analyzer for a multiplane scanner, 109
Kowalsky, R.J., Johnston, R.E., and Chan, F.H. Dose calibrator performance and quality control, 35
Kuhn, S.A. Relocating a nuclear medicine laboratory, 111*

Lands, E.L. ^{67}Ga camera imaging spectrometry, 108*
Lands, E.L. see Brown, T.
LaRocque, L.R. Case of the quarter, 163
LaRocque, L.R. Performance methods in a large-volume nuclear medicine department, 143
Leary, M. see Spicer, J.A.
Leeper, M.A. see Koester, L.M.
Lis, G., Zu'bi, S.M., Sullivan, J.P., and Brahmaver, J.P. Image quality enhancement in pancreas scanning, 108*
Loberg, M. see Sorandes, T.

Mack, B.A., Borer, J.S., Green, M.V., Bacharach, S.L., and Johnston, G.S. ECG-gated rest and stress heart studies, 112*
Maitland, D. see Hambright, P.
Malmud, L.S., Fisher, R.S., Capuzzi, J.P., Grabowski, C., and Charkes, N.D. The acidified gastroesophageal scintiscan, 113*
Manspeaker, H. see Raab, E.
Martin, N.L. Book review: *Xeroradiography: Uncalcified Breast Masses,* 221
McCormick, M.V., Wahner, H.W., and Orvis, A.L. Energy window selection for fluorescence thyroid scanning, 108*
McIlmoyle, G. Book review: *Atlas of Angiography,* 57
McLean, J.R., and Wise, P. Impurities in a ^{99m}Tc lung imaging kit, 28
McLean, J.R., and Wise, P. Mouse bioassay procedure, 105
Miale, A. see Koorji, A.H.
Mikesell, H.H., Nickoloff, E.L., and Kasecamp, W. Comparison of serum T_3 kits, 110*
Moffat, R.E. Book review: *Roentgenology of the Gallbladder and Biliary Tract,* 221

Moser, K.M. see Sgroi, V.L.

Nickoloff, E. see Raab, E.
Nickoloff, E.L. see Mikesell, H.H.

Ochart, M. see Czerwinski, B.
Orvis, A.L. see McCormick, M.V.

Padellford, L. see Tripses, K.
Panetta, P.F. ^{133}Xe adsorption in charcoal traps, 166
Pavel, D.G.
see Baron, K.
see Zimmer, A.M.
Phelps, M.R. see Spicer, J.A.
Pitt, B. see Raab, E.
Press, H.C. see Hambright, P.
Prestidge, D.J. see Williams, R.C.
Prince, J.R. Goodness-of-fit-tests for counting equipment, 41
Prince, J.R. Reply: statistical behavior of counting equipment, 218
Pritchard, E. Quality assurance of patient care, 197
Pritchard, E.D. Quality assurance of patient care, 111*
Pytlik, L.M., Berger, H.J., Gottschalk, A., and Zaret, B.L. ^{201}Tl and ^{99m}Tc-pyrophosphate imaging in acute myocardial infarction, 112*

Quinlan, J. see Sorandes, T.

Raab, E., Nickoloff, E., Manspeaker, H., Pitt, B., and Wagner, H. Dynamic heart model for ventricular time activity curves, 109*
Reese, L. see Wilkins, K.
Rerych, S.K. See Bates, B.B.
Rhodes, B.A.
see Hladik, W.B.
see Spicer, J.A.
see Wells, L.D.
Rich, D.A., Dhawan, V.M., Sziklas, J.J., and Spencer, R.P. A computerized subtraction program for ^{67}Ga scanning, 108*
Robinson, R.G. see Wells, L.D.

Samuel, A.M. The tomoscanner with multiangle readout method, 109*
Sargent, D. see Kan, M.K.
Schwab, C. see Barat, K.
Sgroi, V.L., and Moser, K.M. ^{125}I-fibrinogen detection of deep venous thrombosis, 113*
Shepard, J. see Timpe, G.M.
Shuler, S.E. see Witherspoon, L.R.
Sorandes, T. Model infection control plan, 110*
Sorandes, T. $^{99m}TcO_4^-$ thyroid uptake, 113*
Sorandes, T., Quinlan, J., and Loberg, M. ^{131}I- and ^{125}I-fibrinogen for monitoring renal allografts, 114*
Spencer, R.P. see Rich, D.A.
Spicer, J.A., Phelps, M.R., Leary, M., Callahan, L., and Rhodes, B.A. Radiopharmacy redesign, 90
Stankiewicz, C.J., Giga, J.L., and Carretta, R.F. Technical aspects of hepatic scintiangiography, 155
Stankiewicz, C.J., Giga, J.L., Weiland, F.L., and Carretta, R.F. Simultaneous dual isotope Schilling test, 113*
Steidley, K.D. Book review: *An Introduction to the Physics of Nuclear Medicine,* 171
Steidley, K.D. Book review: *NCRP Report No. 49: Structural Shielding Design and Evaluation for Medical Use of X-rays and Gamma Rays of Energies up to 10 MeV,* 107
Steinman, S. Impurities in a ^{99m}Tc lung imaging kit, 55
Stephan, A. VOICE program, 56
Study, K.T. see Hladik, W.B.
Sullivan, J.P. see Lis, G.
Sziklas, J.J. see Rich, D.A.

Tauxe, W.N. see Kontzen, F.N.
Thorson, L.M., Becker, G.P., and Wahner, H.W. Increased specificity of Ga scans by liver subtraction technique, 114*
Timpe, G.M. ^{133}Xe adsorption in charcoal traps, 167
Timpe, G.M., Deville, T., and Shepard, J. Dose calibrator performance, 169
Tobin, M. see Kontzen, F.N.
Tripses, K., Clark, N., Kirchhoff, K., and Padellford, L. Human serum ferritin assay kit, 110*

Volz, E.M., and Christian, P.E. Case of the quarter, 215

Wagner, H. see Raab, E.
Wagner, H.N. Book review: *Scintillation Camera Lung Imaging, An Anatomic Atlas and Guide,* 106
Wahner, H.W.
see McCormick, M.V.
see Thorson, L.M.
Washburn, R., Dalton, J., Brahmaver, S.M., and Zu'bi, S.M. Quality control and target values for radioimmunoassays, 109*
Weiland, F.L. see Stankiewicz, C.J.
Weiss, S., and Conway, J.J. Bone imaging artifacts, 17
Wells, L.D. Letter from the Editor, 15, 142, 193
Wells, L.D., Robinson, R.G., and Rhodes, B.A. Scheduling nuclear medicine and radiographic exams, 111*
Wilkerson, S.V. see Gunther, C.W.
Wilkins, K., and Reese, L. Left ventricular ejection fractions using a multi-crystal scintillation camera, 112*
Williams, J. Prolactin radioimmunoassay, 110*
Williams, R.C., Chilton, H.M., and Prestidge, D.J. Adaptation of a multichannel scaler device for radiochromatogram scanning, 208
Wise, P. see McLean, J.R.
Witherspoon, L.R., Shuler, S.E., and Blonde, L. Rectilinear bone scanning, 23

Zaret, B.L. see Pytlik, L.M.
Zeuske, G. Licensure, 56
Zimmer, A.M., and Pavel, D.G. Stabilized and non-stabilized ^{99m}Tc-Sn-diphosphonate kits, 54
Zimmer, A.M. see Baron, K.
Zu'bi, S.M.
see Lis, G.
see Washburn, R.

1977 Subject Index

(Asterisk indicates abstract)

Artifact
acute myocardial infarction imaging, 112*
bone imaging, ^{99m}Tc-diphosphonate, 17
flood field image, particulate phantom content, 213
liver-spleen image, bladder activity, 163
Biliary, *see Gallbladder*
Bladder
activity on liver-spleen scan, 163
Blood, *see Red blood cells*
Bone
imaging, artifacts, ^{99m}Tc-diphosphonate, 17
imaging, cranial hyperostosis, 161
rib phantom for myocardial studies, 50
scanning, bladder retention of activity, 163
scanning, techniques, ^{99m}Tc-pyrophosphate, 23
^{99m}Tc-diphosphonate kit evaluation, 54
tomography, 146, 152
Book review
An Introduction to the Physics of Nuclear Medicine, 171
Atlas of angiography, 57
ICRU Report 25, Conceptual Basis for the Determination of Dose Equivalent, 106
NCRP Report No. 49: Structural Shielding Design and Evaluation for Medical Use of X-rays and Gamma Rays of Energies up to 10 MeV, 107
Roentgenology of the Gallbladder and Biliary Tract, 221
Scintillation Camera Lung Imaging: An Anatomic Atlas and Guide, 106
The Basic Physics of Radiation Therapy, 2nd Edition, 106
Xeroradiography: Uncalcified Breast Masses, 221
Brain
angiography, book review, 57
imaging, Dandy-Walker cyst, ^{99m}Tc-GHT, in infant, 85
tomography, Anger rectilinear tomographic scanner, 146
tomography, $^{99m}TcO_4^-$, 152
Breast
xeroradiography, uncalcified mass, book review, 221
Camera, scintillation
computer system choice, 199
lung imaging, book review, 106
multi-crystal, left ventricular ejection fraction, 112*
window settings, ^{67}Ga, 108*
window settings, myocardial imaging, 52
Cardiology, *see Heart*
Cesium-137
source, equipment performance testing, 41
Chi-square test, 41, 217, 218
Chromatography
gel column, ^{99m}Tc-agents, 94
miniaturized, ^{99m}Tc-diphosphonate, 54
paper, ^{99m}Tc-MAA, 111*
radio-, scanning device, 208
^{99m}Tc-Sn-MAA, 28
Chromium-51
red blood cell labeling syringe, 32
Clinical evaluation
Anger rectilinear tomographic scanner, 146
ferritin radioassay, 63 cases, 110*
myocardial imaging, acute infarct, technical aspects, 385 cases, 112*
pancreas scanning, cold spot technique, 720 cases, 108*
prolactin radioimmunoassay, 110*
T_3 kits, 109 cases, 110*
Computer
^{67}Ga/^{99m}Tc subtraction technique, 108*
systems, buyer's guide, 199
Departmental operations
department design, 112*
emergency planning, 46
infection control, 110*
laboratory relocation, 111*
large volume scheduling, performance control, 143
quality assurance of patient care, 111*, 197
radiopharmacy design, 90
record keeping, 143
scheduling, nuclear medicine and radiography studies, 111*
Diphosphonate, *see Technetium-99m*
Display
choice of, 199
Dose calibrator
performance, quality control, 35, 168, 169
Education
book review: physics of nuclear medicine, 171
in-service, 169
VOICE program, 56
Field uniformity
Anger rectilinear tomographic scanner, 146
effect of phantom contents, 213
Fluorescence scanning
thyroid, energy window selection, 108*
Folate
radioassay, normal range, 101
radioimmunoassay, normal values, 101
radioimmunoassay, quality assurance, 109*
Gallbladder
roentgenology, book review, 221
Gallium-67
camera window settings, 108*
^{99m}Tc image subtraction, 108*
tomography, Anger rectilinear scanner, 146
tomography, dual photopeak analyzer, 109*
Gastrointestinal tract
reduced Tc uptake, in animals, 110*
Gating
ECG, 112*
Heart
dynamic model, ventricular time–activity curves, 109*
ECG-gated studies, rest and stress, 112*
exercise studies, ^{99m}Tc, 112*
imaging, rib phantom, 50
imaging, ^{99m}Tc-albumin, window setting, 52
imaging, ^{201}Tl, ^{99m}Tc-pyrophosphate, 112*
left ventricular ejection fraction, multi-crystal scintillation camera, 112*
Hippuran, *see Iodine-131*
Infection
control, 110*
Instrumentation, *see specific instrument*
Insulin
radioimmunoassay kit improvement, 205
Iodine-125
dose calibrator performance, 35
-insulin, radioimmunoassay kit, 205
Iodine-131
dose calibrator performance, 35, 168, 169
-o-iodohippurate, comprehensive renal function studies, 81
Kidney
screening study, imaging, urinary excretion, ERPF, ^{131}I-o-iodohippurate, 81
Kit
ferritin assay, 110*
insulin radioimmunoassay, improvement, 205
Serum T_3, comparison, 110*
^{99m}Tc-diphosphate, evaluation, 54
^{99m}Tc, radiochromatogram scanning, 208
^{99m}Tc-Sn-MAA, impurities, 28, 55, 105
^{99m}Tc, Sn(II) spot test, 88
Kolmogrov-Smirnov test, 41, 217, 218
Lexis' divergence coefficient, 41, 217, 218
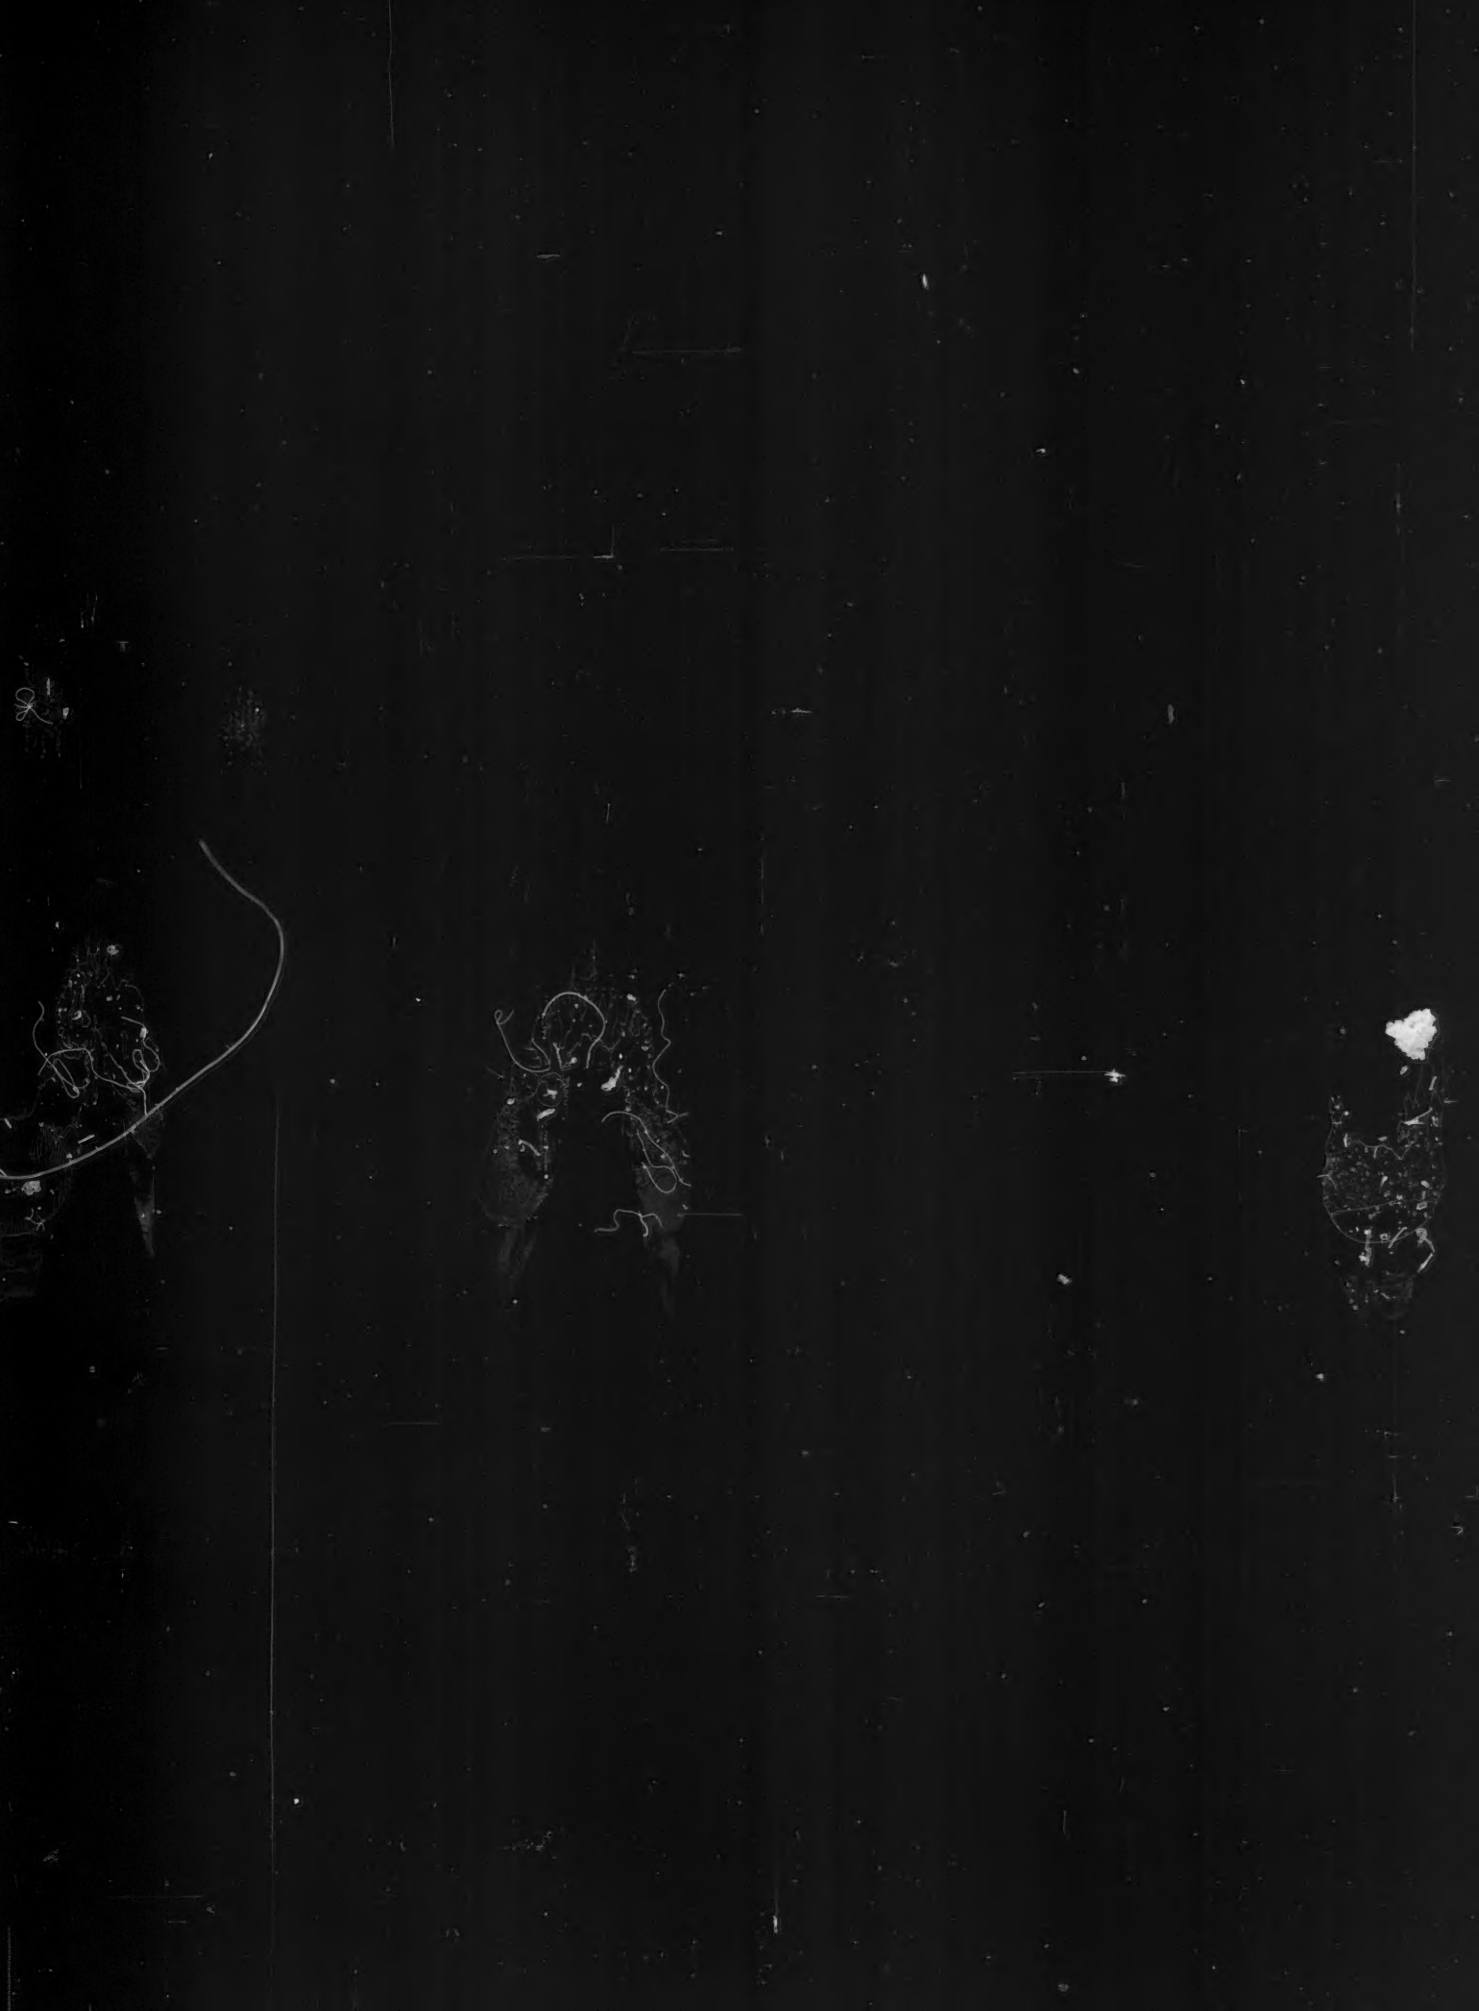
Licensure
Technologist Section SNM Position Paper, 56
Liver
imaging, bladder activity, 163
reduced Tc uptake, in animals, 110*
scintiangiography, ^{99m}Tc-S colloid, 155
Lung
CO_2 rebreathing effects, correction, 211
imaging, book review, 106
studies, ^{133}Xe charcoal trap adsorption, 166, 167
^{99m}Tc-Sn-MAA kit, purity, 28, 55, 105
ventilation and perfusion, right-to-left shunt, ^{133}Xe, ^{99m}Tc-MAA, 215
Models
animal, tissue distribution, 55, 105
heart, dynamic, ventricular time–activity curves, 109*
Myocardial, *see Heart*
o-iodohippurate, *see Iodine-131*
Pancreas
scanning, cold spot technique, image subtraction, 108*
Patient
comfort, 197, 211
position, liver scintiangiography, 155
Pediatrics
Dandy-Walker cyst, brain imaging, ^{99m}Tc-GHT, 85
Pertechnetate, *see Technetium-99m*
Phantom
emission tomography, 109*
flood field uniformity, artifact, 215
rib, myocardial studies, 50
tomographic, 109*
Pituitary gland
adenoma, prolactin radioimmunoassay, 110*
Prolactin
radioimmunoassay, clinical applications, 110*
Pyrophosphate, *see Technetium-99m*
Quality control
dose calibrator, 35, 168, 169
equipment, goodness-of-fit test, 41, 217, 218
flood field phantom content, 213
folate radioimmunoassay, 109*
radiochemical, rapid feedback system, 94
Sn(II) spot test, 88
^{99m}Tc-diphosphonate kit evaluation, 54
^{99m}Tc-MAA, commercial, 111*
^{99m}Tc-MAA kit, 28, 55, 105
^{99m}Tc-MAA, labeling efficiency tests, 217
Radiation dosimetry
dose equivalent determination, book review, 106
Radiation safety
accident management, 46
charcoal trap adsorption of ^{133}Xe, 166, 167
hand exposure, 158
liver scintiangiography studies, ^{99m}Tc, 155
shielding, book review, 107
Radiation therapy
basic physics, book review, 106
Radioassay
ferritin, kit evaluation, 110*
normal range estimation, 101
Radioimmunoassay
folate, quality control, 109*
insulin, kit improvement, 205
prolactin, clinical application, 110*
Radiopharmacy
design, 90
Red blood cells
^{51}Cr, ^{99m}Tc labeling, syringe, 32
Reliability factor
equipment performance test, 41, 217, 218
Scaler
multichannel, radiochromatogram scaling, 208
Scanner
tomographic multiplane, 152
Scanner, rectilinear
Anger, tomographic, 146
bone-scanning techniques, ^{99m}Tc-pyrophosphate, 23
^{67}Ga-citrate study, compared to tomographic scanner, 146
Selenium-75, selenomethionine
pancreas scanning, cold spot technique, 108*
Skull
cranial hyperostosis, bone imaging, 161
Spleen imaging
bladder activity, 163
Technetium-99m
-agents, quality control, rapid feedback system, 94
-albumin, myocardial imaging, 52
angiocardiography, exercise, 112*
-diphosphonate, bone imaging artifacts, 17
-diphosphonate, bone tomography, 146
-diphosphonate, kit evaluation, 54
dose calibrator performance, 35, 168, 169
-GHT, brain imaging, in infant, 85
-gluconate, left ventricular ejection fraction, 112*
image subtraction, ^{67}Ga scanning, 108*
kit preparation, radiochromatogram scanning, 208
kits, Sn(II) spot test, 88
-MAA, commercial, evaluation, 111*
-MAA, lung perfusion, right-to-left shunt, 215
-MAA, particle number effects, 215
pertechnetate, brain tomography, 146
-pyrophosphate, acute myocardial infarction imaging, 112*
-pyrophosphate, bone-scanning techniques, 23
-pyrophosphate, myocardial studies, rib phantom, 50
reduced, effect on imaging, in animals, 110*
-red blood cells, labeling syringe, 32
-S colloid, liver image subtraction, pancreas scanning, 108*
-S colloid, liver–spleen imaging, bladder activity, 163
-S colloid, scintiangiography, 155
-Sn-MAA, kit, purity, 28, 55, 105
Thallium-201
heart imaging, acute infarction, 112*
Thyrotropin
radioassay, normal range, 101
Thyroid
fluorescence scanning, window selection, 108*
Thyroxine
CPB, normal range, 101
Tomography
Anger rectilinear tomographic scanner, 146
clinical experience, 109*
dual independent, photopeak analyzer, 109*
multiangle readout, 109*
plane distribution, 152
Training, *see Education*
TSH, *see Thyrotropin*
Tumor
breast mass, uncalcified, xeroradiography, book review, 221
T_3
kits, comparison, 100*
uptake, normal range, 101
T_4, *see Thyroxine*
Vitamin B_{12}
radioassay, normal range, 101
Xenon-133
charcoal trap adsorption, 166, 167
lung ventilation, right-to-left shunt, 215
Xeroradiography
uncalcified breast mass, book review, 221
X-ray
gallbladder, biliary tract, 221
studies, scheduling with nuclear medicine, 111*